


CM-Series Spectrophotometer (Sample)

KONICA MINOLTA, INC.
Sensing Business Unit
Quality Assurance Division

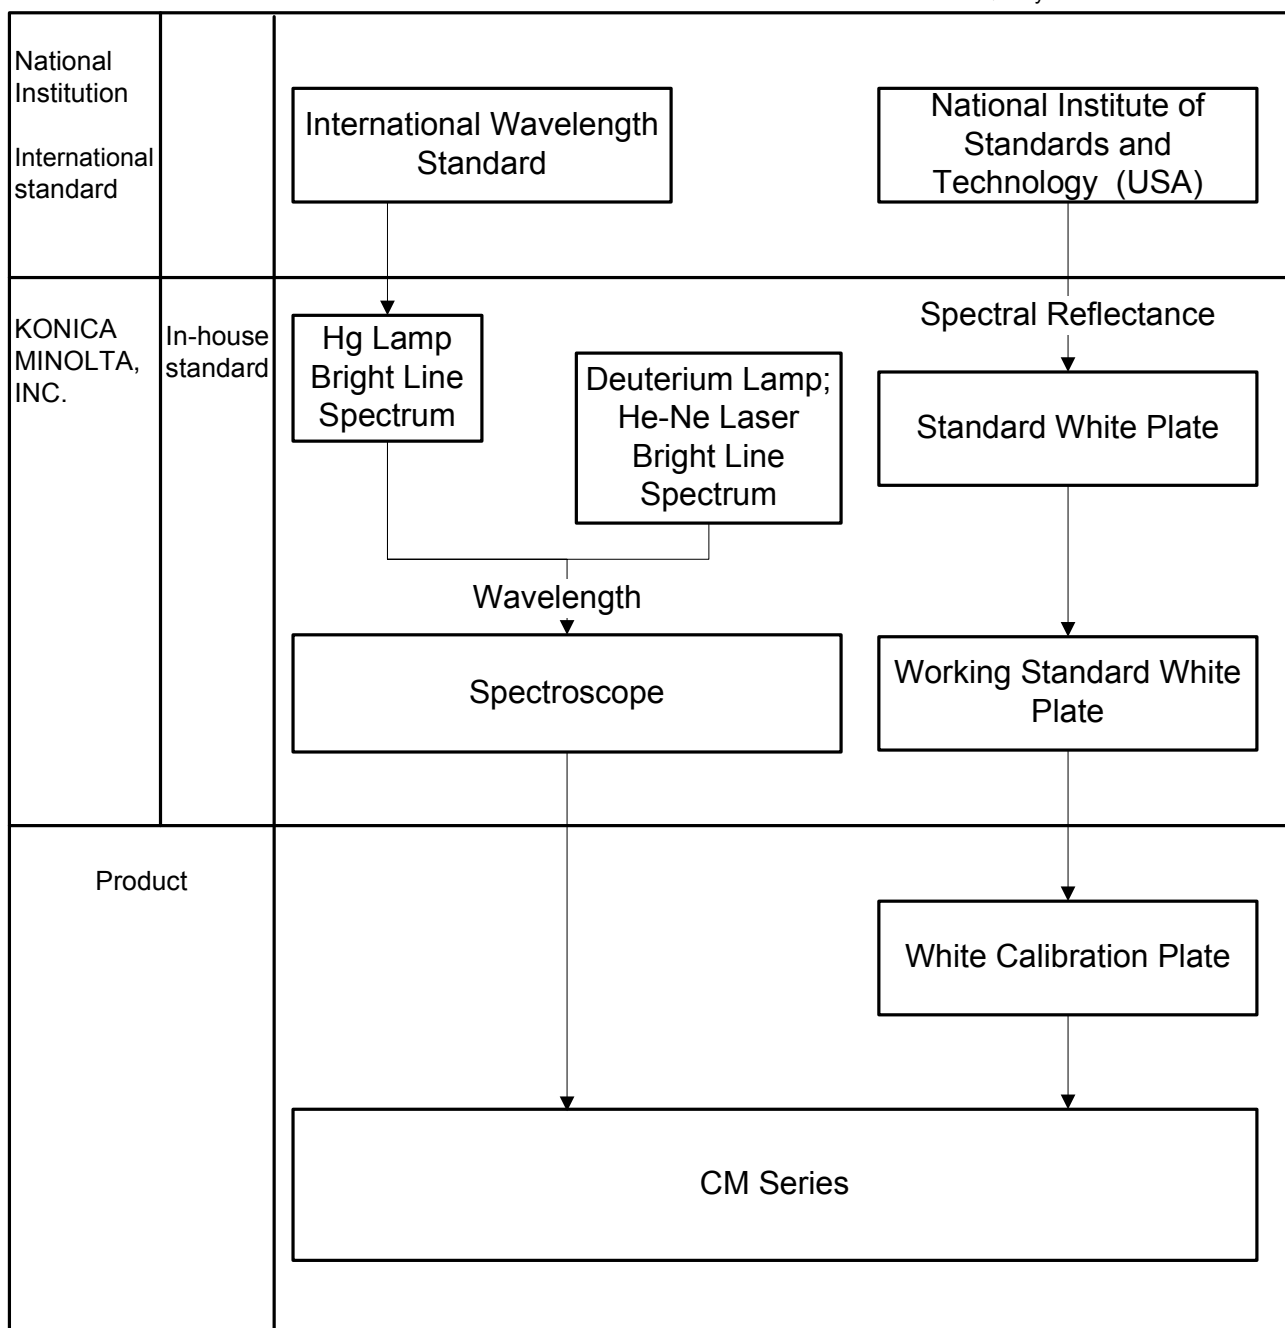

Interval between calibration:

Spectroscope: 1 year

Standard White Plate: 5 years

Working Standard White Plate: 1 year