



KONICA MINOLTA

# Skin Analysis Software CM-SA

6

For quantitative evaluation & analysis of skin color and pigmentation

## Simultaneous Measurement of Skin Color and Melanin Index

Used in combination with a Konica Minolta spectrophotometer, the CM-SA enables highly accurate measurement of skin color simultaneously with a numerical display of the Melanin Index, Hb (Hemoglobin) Index, and Hb SO<sub>2</sub> (Hemoglobin oxygen saturation) Index (%).



For applications in the R&D divisions of cosmetic, functional food, and pharmaceutical companies developing products with “skin-lightening” effects, commissioned clinical testing organizations, and research institutes for dermatology, plastic surgery, etc.


# Realizing Simultaneous Measurement of Skin Color and Melanin Index!

In the field of skin research and development, there is an increasing demand to measure the color and pigmentation of skin as it provides valuable information on a number of factors. For example, where cosmetics are concerned companies are aiming to make products that more closely match or complement the skin tone of clients. In pharmaceutical research and development, skin measurement can be used to determine the effects of suntanning on skin and in the prevention of sunburn.


The software provides important factors of skin data: color, melanin, hemoglobin and oxygen saturation. This software employs an original algorithm to separately calculate Melanin Index, Hb Index, and Hb SO<sub>2</sub> Index (%) based on the spectral reflectance data measured by a spectrophotometer, enabling highly accurate measurement of melanin pigmentation level of the skin without being affected by skin redness.

## Combining the Melanin Measurement Function with a Spectrophotometer


By using this software in combination with a spectrophotometer, Melanin Index, Hb Index, and Hb SO<sub>2</sub> Index can be measured simultaneously with spectral reflectance and colorimetric values in a single operation. There is no need to separately measure the color of skin and Melanin Index using different instruments, as was previously necessary.

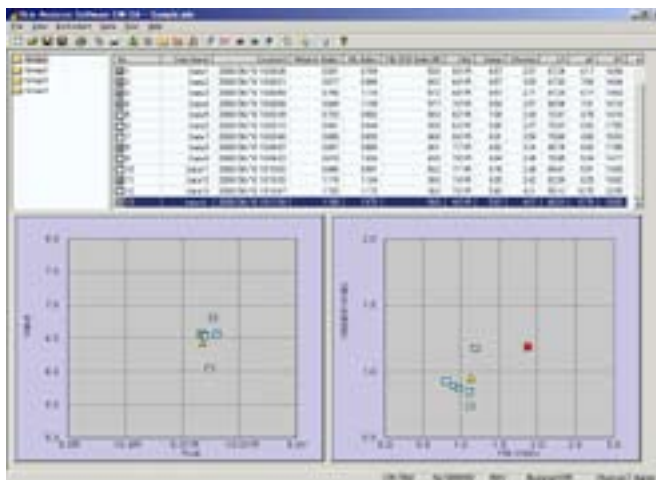

**Hb Index–Melanin Index Graph**

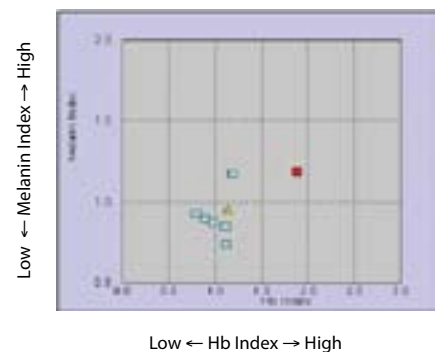

**Munsell Hue–Value Graph**

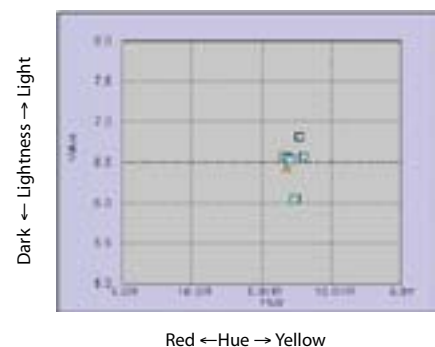

# The handheld CM-700d/CM-600d enables simple operations while standing.

## Simple measurement

Measurement can be performed by simply placing the head of spectrophotometer against the skin and pressing the button. Measurement by just applying light to the face, arm, or other desired part of the body will not put undue stress on the examinees.



## Featuring Bluetooth®

The Bluetooth® function of Spectrophotometer CM-700d/CM-600d enables wireless transmission of measured data to the PC, offering greater flexibility for measurements without the constraints of communication cables.

Can be used for consecutive measurements, enabling efficient measurements of a number of examinees.

(Useful for applications at laboratory testing institutes)

## Data can be easily grouped by examinee

The CM-SA features a function to automatically switch groups by examinee. When a preset number of measurements is reached, the next measurement data can be linked to the next group.


(Useful for consecutive measurements on a number of examinees)

### Example

When there are Examinees 1, 2, and 3, and the number of measurements is set to 3, the group is automatically changed to the next one every three measurements, and the data is linked to the relevant group (examinee).

## Output of measured data in CSV text format

The measurement results can be output in CSV text format to be utilized for further analysis or data management using Excel® or other spreadsheet applications.

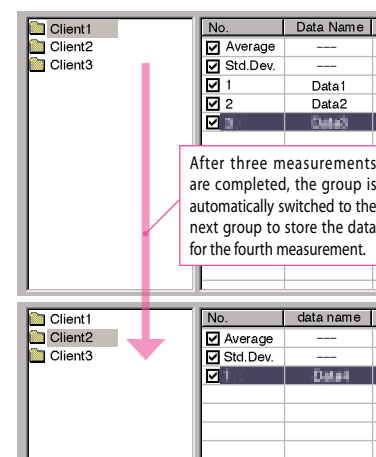

No.	Data Name
<input checked="" type="checkbox"/>	Average
<input checked="" type="checkbox"/>	Std.Dev.
<input checked="" type="checkbox"/>	1 Data1
<input checked="" type="checkbox"/>	2 Data2
<input checked="" type="checkbox"/>	3 Data3

After three measurements are completed, the group is automatically switched to the next group to store the data for the fourth measurement.

No.	data name
<input checked="" type="checkbox"/>	Average
<input checked="" type="checkbox"/>	Std.Dev.
<input checked="" type="checkbox"/>	1 Data1



## <Major specifications of CM-SA>

Skin data display	Melanin Index Hb Index [Total hemoglobin (oxidized + reduced) index] Hb SO <sub>2</sub> Index (%) [Hemoglobin oxygen saturation index (%)]
Colorimetric data display	L*, a*, b*, Munsell value (Hue, Value, Chroma) <sup>*1</sup>
Graph display	Hue-Value Graph, Hb Index-Melanin Index Graph
Data handling	Saving/reading data in CM-SA original format Saving data in text (CSV) format [Melanin Index, Hb Index, Hb SO <sub>2</sub> Index (%), L*, a*, b*, Munsell value (Hue, Value, Chroma), Spectral reflectance (400-700 nm) <sup>*2</sup> ]

\*1 Munsell data are calculated for 2° observer and Standard Illuminant C.

\*2 The spectral reflectance data that are output are the reflectance obtained in SCI (specular component included) mode.

## <PC operating environment>

OS	Windows® 7 Professional 32-bit, 64-bit, Windows® 8.1 Pro 32-bit, 64-bit, Windows® 10 Pro 32-bit, 64-bit <small>*The hardware of the computer system to be used must meet or exceed the greater of the recommended system requirements for the compatible OS being used or the following specifications.</small>
CPU	Pentium® III 600 MHz or equivalent (recommended)
Memory	128 MB or more (256 MB or more is recommended)
Hard disk	100 MB or more free disk space is required.
Display	Display capable of displaying 1,024 × 768 pixels or above/16-bit color or above
Other	CD-ROM drive (required for software installation), USB port or serial port (required for connecting the PC with the instrument)

## <Main specifications of compatible spectrophotometers>

\* Some instrument functions not available when using instrument with CM-SA.

Model	CM-700d	CM-600d	CM-2600d	CM-2500d
Wavelength range	400 nm to 700 nm		360 nm to 740 nm	
Wavelength pitch	10 nm			
Light source	Pulsed xenon lamp (with UV cut filter)		Pulsed xenon lamp	
Measurement time	Approx. 1 second		Approx. 1.5 seconds (Approx. 2 seconds for fluorescent measurement)	Approx. 1.5 seconds
Minimum measurement interval	Approx. 2 seconds for SCI or SCE measurement		3 seconds for SCI/SCE measurement (4 seconds for fluorescent measurement)	3 seconds for SCI/SCE measurement
Battery performance (max. measurement count)	Approx. 2,000 measurements with alkaline dry batteries Approx. 2,000 measurements with fully charged nickel-metal-hydrate rechargeable batteries (2300 mAh) <small>*Continuous measurements at 10-second intervals at 23°C (single measurement fixed at SCI or SCE)</small>		Approx. 1,000 measurements with alkaline dry batteries <small>*Continuous measurements at 10-second intervals at 23°C</small>	
Measurement/illumination area	MAV : Ø8 mm/ Ø11 mm SAV : Ø3 mm/ Ø6 mm <small>*Changeable by replacing target mask and selecting lens position</small>	MAV : Ø8 mm/ Ø11 mm only	MAV : Ø8 mm/ Ø11 mm SAV : Ø3 mm/ Ø6 mm <small>*Changeable by replacing target mask and selecting lens position</small>	MAV : Ø8 mm/ Ø11 mm only
Repeatability	Spectral reflectance: Standard deviation within 0.1% Colorimetric value: Standard deviation within $\Delta E^*ab$ 0.04 <small>*When a white calibration plate is measured 30 times at 10-second intervals after white calibration</small>		Spectral reflectance: Standard deviation within 0.1% (standard deviation within 0.2% for the wavelength range of 360 to 380 nm) Colorimetric value: Standard deviation within $\Delta E^*ab$ 0.04 <small>*When a white calibration plate is measured 30 times at 10-second intervals after white calibration</small>	
Inter-instrument agreement	Within $\Delta E^*ab$ 0.2 (MAV/SCI) *Average of 12-color measurement with the BCRA Series II compared to values measured with a master body at 23°C			
No. of averaging measurements	1 to 10 measurements (automatic averaging); 1 to 30 measurements (manual averaging)		1/3/5/8 measurements (automatic averaging); 1 to 30 measurements (manual averaging)	
Interface	USB1.1 and Bluetooth® standard version 1.2*		RS-232C-compliant	
Power	4 AA-size alkaline dry batteries or nickel-metal-hydrate rechargeable batteries; Special AC adapter			
Size	73 (W) × 211.5 (H) × 107 (D) mm		69 (W) × 96 (H) × 193 (D) mm	
Weight	Approx. 550 g (without white calibration cap and batteries)		Approx. 670 g (with Measuring Base/without batteries)	

\* Applicable Bluetooth® profile: Serial Port Profile, Output: Bluetooth® Power Class 1

The communication distance may vary depending on the obstacles and radio wave conditions between the devices.

Successful wireless communication is not guaranteed with all Bluetooth®-ready equipment.

- Bluetooth® is a registered trademark of The Bluetooth SIG, Inc. and is used under license agreement.
- Windows® is a trademark or registered trademark of Microsoft Corporation in the U.S.A. and other countries.
- Pentium® is a trademark or registered trademark of Intel Corporation in the U.S.A. and other countries.
- The specifications shown herein are subject to change without notice.
- KONICA MINOLTA, the Konica Minolta logo and symbol mark, and "Giving Shape to Ideas" are registered trademarks or trademarks of Konica Minolta, Inc.



### SAFETY PRECAUTIONS

For correct use and for your safety, be sure to read the instruction manual before using the instrument.



Certificate No.: JQA-QMA15888  
Registration Date: October 26, 2018  
KONICA MINOLTA, Inc., Sakai Site  
Product design, manufacture/manufacturing management, calibration, and service



Certificate No.: JQA-E-80027  
Registration Date: March 12, 1997  
KONICA MINOLTA, Inc., Sakai Site

#### KONICA MINOLTA, INC.

Konica Minolta Sensing Americas, Inc.  
Konica Minolta Sensing Europe B.V.

Osaka, Japan  
New Jersey, U.S.A.  
European Headquarter /BENELUX  
German Office  
French Office  
UK Office  
Italian Office  
Swiss Office  
Nordic Office  
Polish Office  
Turkish Office  
SE Sales Division  
Beijing Office  
Guangzhou Office  
Chongqing Office  
Qingdao Office  
Wuhan Office

Phone : 888-473-2656 (in USA), 201-236-4300 (outside USA)  
Nieuwegein, Netherlands Phone : +31 (0) 30 248-1193  
München, Germany Phone : +49 (0) 89 4357 156 0  
Roissy CDG, France Phone : +33 (0) 1 80 11 10 70  
Warrington, United Kingdom Phone : +44 (0) 1925 467300  
Cinisello Balsamo, Italy Phone : +39 02849488.00  
Dietikon, Switzerland Phone : +41 (0) 43 322-9800  
Västra Frölunda, Sweden Phone : +46 (0) 31 7099464  
Wrocław, Poland Phone : +48 (0) 71 73452-11  
Istanbul, Turkey Phone : +90 (0) 216-528 56 56  
Shanghai, China Phone : +86- (0)21-5489 0202  
Beijing, China Phone : +86- (0)10-8522 1551  
Guangdong, China Phone : +86- (0)20-3826 4220  
Chongqing, China Phone : +86- (0)23-6773 4988  
Shandong, China Phone : +86- (0)532-8079 1871  
Hubei, China Phone : +86- (0)27-8544 9942  
Singapore Phone : +65 6563-5533  
Goyang-si, Korea Phone : +82 (0) 2-523-9726

Fax : 201-785-2482  
Fax : +31 (0) 30 24 81 211  
Fax : +49 (0) 89 4357 156 99  
Fax : +33 (0) 1 80 11 10 82  
Fax : +44 (0) 1925 711143  
Fax : +39 02849488.30  
Fax : +41 (0) 43 322-9809  
Fax : +48 (0) 71 734 52 10  
Fax : +90 (0) 212-253 49 69  
Fax : +86- (0)21-5489 0005  
Fax : +86- (0)10-8522 1241  
Fax : +86- (0)20-3826 4223  
Fax : +86- (0)23-6773 4799  
Fax : +86- (0)532-8079 1873  
Fax : +86- (0)27-8544 9991  
Fax : +65 6560-9721  
Fax : +82 (0) 31-995-6511

#### Konica Minolta (CHINA) Investment Ltd.

Konica Minolta Sensing Singapore Pte Ltd.  
Konica Minolta Sensing Korea Co., Ltd.

Addresses and telephone/fax numbers are subject to change without notice. For the latest contact information, please refer to the KONICA MINOLTA Worldwide Offices web page :

<https://konicaminolta.com/instruments/network>