



KONICA MINOLTA

Spectrophotometer CM-5

An advanced all-in-one spectrophotometer with innovative operation to let anyone take measurements easily anytime



The CM-5 makes color measurements simple. Just switch it on and start taking measurements. No need to bother with a computer; the CM-5 has a full range of advanced functions including specialized indices for a variety of applications and a large color display that makes results easy to read.

Finally, high accuracy and ease of use in a compact top-port spectrophotometer!

Measurements as simple as 1-2-3!



Switch on power.

The CM-5 starts up and **automatically performs white/100% calibration*** using an internal white calibration plate behind the shutter.

* Not applicable to liquid transmittance measurements using cells.



Position sample.


For reflectance, the **top port** makes measuring samples of various shapes and sizes easy. For transmittance, sliding open the CM-5 reveals a **large transmittance chamber**. Liquids can be measured using optional cells.



Press MEAS.

The measurement is taken and the results appear in the display. The **large color LCD** enables data to be shown not only numerically, but also on the colorimetric plots and spectral graphs that normally require a computer to display.

Actual CM-5 screens!

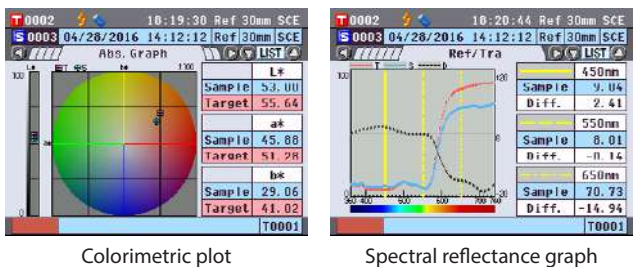


Colorimetric plot

Spectral reflectance graph

Screens can be shown in any of **8 languages**: English, Japanese, German, French, Italian, Spanish, Simplified Chinese, and Portuguese.

Just follow the wizard!

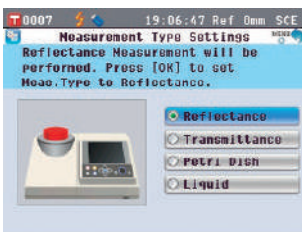

Even beginners can take measurements easily without mistakes.

The CM-5's **wizard mode** guides users through each step, helping users to make settings and take measurements without having to get out the instruction manual each time.

Avoid multi-user confusion with USB!

The CM-5 lets users store their own settings on their own USB memory stick, so they can restore the settings they need by simply reading them from the memory stick instead of redoing settings individually.




Enter text directly with a USB keyboard *

You can connect a USB keyboard * to the CM-5 to enter text directly when editing data names and comments.

*Keyboard layout: US keyboard layout



System Diagram

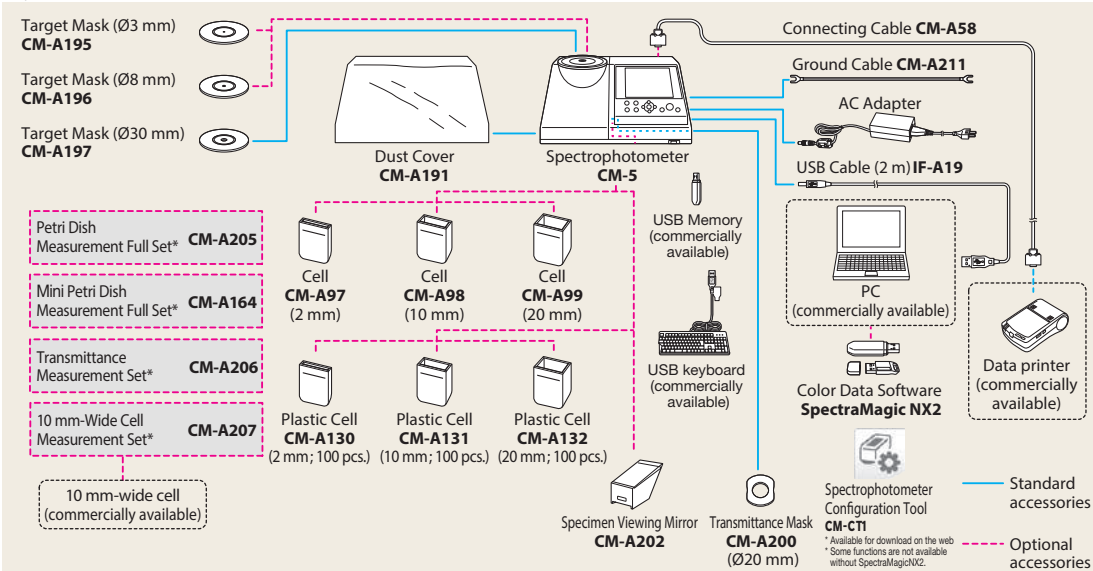

* For details, refer to the following table. Mini Petri Dish CM-157 requires firmware version 1.2 or later.

	Petri Dish Measurement Full Set CM-A205	Mini Petri Dish Measurement Full Set CM-A164	Transmittance Measurement Set CM-A206	10 mm-Wide Cell Measurement Set CM-A207
White Calibration Plate (with CD-ROM containing calibration data and data-setting software)	○	○		
Zero Calibration Box	○	○		
Target Mask (for Petri Dish)	○			
Petri Dish	○			
Calibration Glass (for Petri Dish)	○			
Target Mask (for Mini Petri Dish)		○		
Mini Petri Dish		○		
Calibration Glass (for Mini Petri Dish)		○		
Transmittance Zero Calibration Plate			○	
Transmittance Specimen Holder			○	
Transmittance Specimen Holder Attachment			○	
Transmittance Specimen Holder (10 mm-wide cells)				○
Transmittance Zero Calibration Plate (10 mm-wide cells)				○
Accessory Case	○	○	○	



Petri Dish Measurement Full Set CM-A205



Mini Petri Dish Measurement Full Set CM-A164



Transmittance Measurement Set CM-A206



10 mm-Wide Cell Measurement Set CM-A207

Compact, versatile color instrument


Reflectance measurements

The measuring port of the CM-5 is on top, so users can just place a solid object on the port and press the MEAS. button. There's no need to clamp the sample in a sample holder, and there's no worry about the sample shifting position. And, by using a Petri dish (optional accessory), liquids, pastes, and powders can also be measured easily.

Samples are just placed on top, so even large samples can be measured.



By using the Ø3 mm target mask (optional accessory), even small samples can be measured.



Pastes can also be measured using a Petri dish (optional accessory).




Colorant pellets can be measured in raw form using a Petri dish (optional accessory).



Ø16 mm Mini Petri Dish for small sample amounts* (Optional accessory)

The optional Mini Petri Dish enables measurements of costly powder samples such as rare-earth metals, organic EL materials, pharmaceuticals, etc. to be taken using much less sample material (approximately 1/20 of amounts required using our conventional Petri Dish CM-A128). In addition, the automatic white calibration function also works with the Mini Petri Dish, so measurements can be taken shortly after switching the instrument on without performing calibration manually.


* This optional accessory can be used with firmware version 1.2 or later.



Transmittance measurements

The CM-5's transmittance chamber is large and sideless, enabling measurements of even large sample sheets with thicknesses up to 60 mm.

For liquids, optional cells with 3 optical path lengths for different sample densities are available, and commercial 10 mm-wide cells can also be used.

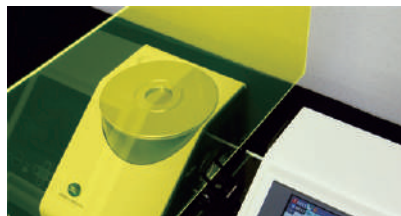

Internal calibration curves for measuring standard chemical/pharmaceutical indices

The CM-5 can measure several of the standard color indices commonly used in the chemical and pharmaceutical field: Gardner, Platinum-Cobalt Color Scale (Hazen/ APHA), Iodine Color Number, European Pharmacopoeia, US Pharmacopoeia and Japanese Pharmacopoeia. Calibration curves for these indices are stored in the CM-5, so measurements of samples based on these indices can be performed quickly and easily by anyone.



* Index calibration curves were measured using 10 mm-Wide Cell Measurement Set CM-A207 and commercially available 10 mm-wide cells with 10 mm optional path length.

* APHA display range: 0 to 1000; Gardner display range: 0 to 18

Spectral absorbance measurements


Spectral absorbance can now be measured and displayed numerically or graphically, enabling evaluation of spectral absorbance for checking absorbance wavelengths, evaluating colorants, calculating K/S, determining components, etc.

Main Specifications

Model	Spectrophotometer CM-5		
Illumination/viewing system	Reflectance:	di:8°, de:8° (diffuse illumination: 8° viewing)	
		SCI (specular component included)/SCE (specular component excluded) switchable	
		Conforms to CIE No. 15 (2004), ISO 7724/1, ASTM E 1164, DIN 5033 Teil 7, and JIS Z 8722 condition c standard.	
	Transmittance:	di:0°, de:0° (diffuse illumination: 0° viewing)	
Conforms to CIE No. 15 (2004), ASTM E 1164, DIN 5033 Teil 7, and JIS Z 8722 condition g standard.			
Integrating sphere size	Ø152 mm		
Detector	Dual 40-element silicon photodiode arrays		
Spectral separation device	Planar diffraction grating		
Wavelength range	360 nm to 740 nm		
Wavelength pitch	10 nm		
Half bandwidth	Approx. 10 nm		
Measurement range	0 to 175 % (Reflectance or transmittance); Output/display resolution: 0.01%		
Light source	Pulsed xenon lamp		
Measurement time	Approx. 1 s (to data display/output); Minimum measurement interval: Approx. 3 s		
Measurement/Illumination area	Reflectance:	Changeable by changing mask and settings. LAV: Ø30 mm/Ø36 mm; MAV (optional): Ø8 mm/Ø11 mm; SAV (optional): Ø3 mm/Ø6 mm	
	Transmittance:	Approx. Ø20 mm/ Ø26 mm	
Repeatability	Spectral reflectance: Standard deviation within 0.1% (400 nm to 740 nm) Chromaticity value: Standard deviation within ΔE*ab 0.04 (When a white calibration plate is measured 30 times at 10-second intervals after white calibration)		
Inter-instrument agreement	Within ΔE*ab 0.15 (Typical) (LAV/SCI) (Based on 12 BCRA Series II color tiles compared to values measured with a master body under Konica Minolta standard conditions)		
Transmittance chamber	No sides (unlimited sample length); Depth (maximum sample thickness): 60 mm Sample holders (optional) for holding sheet samples or containers of liquid samples can be installed/removed		
Display	5.7-inch TFT color LCD		
Display languages	English, Japanese, German, French, Italian, Spanish, Simplified Chinese, Portuguese		
White/100% calibration	Automatic white (reflectance)/100% (transmittance) calibration using internal white calibration plate (Not applicable to 100% calibration when using cells for transmittance measurements of liquids.)		
Interfaces	USB 1.1(Connection to PC, USB memory *1, USB keyboard *2); RS-232C standard (Connection to serial printer)		
Observer	2° or 10° Standard Observer		
Illuminant	A, C, D50, D65, F2, F6, F7, F8, F10, F11, F12, ID50, ID65 (simultaneous evaluation with two light sources possible)		
Displayed data	Spectral values/graph (reflectance, transmittance, absorbance) , colorimetric values/graph, color-difference values/graph, pass/fail judgment, pseudocolor, color assessment		
Colorimetric data	L*a*b*, L*C*h, Hunter Lab, Yxy, XYZ, and color differences in these spaces; Munsell		
Indexes	Reflectance:	MI; WI (ASTM E 313-73, ASTM E 313-96, Hunter); YI (ASTM E 313-73, ASTM E 313-96, ASTM D 1925); WB (ASTM E 313-73); ISO Brightness	
	Transmittance:	Gardner; Iodine Color Number; Platinum-Cobalt Color Scale (Hazen/ APHA); European Pharmacopoeia; US Pharmacopoeia	
User index	User-defined index (Optional CM-CT1(Ver.1.4 or later) and Color Management Software SpectraMagic™ NX2 required for setting user index.) * User index can be used with CM-5/CR-5 firmware version 1.2 or later.		
Color-difference equation	ΔE*ab (CIE 1976), ΔE*94 (CIE 1994), ΔE00 (CIE DE2000), ΔE (Hunter), CMC (l: c)		
Pass/Fail judgment	Tolerances can be set to colorimetric values (except Munsell), color-difference values, or reflectance index values		
Data memory	Measurement data: 4,000 measurements; Target color data: 1,000 measurements		
USB memory*1 storage	Storage of measurement data and target color data. Storage/reading of measurement condition settings		
Power	AC 100 to 240 V, 50/60 Hz (using exclusive AC Adapter)		
Size (W × H × D)	Slide cover closed: 385 × 192 × 261mm Slide cover open: 475 × 192 × 261 mm		
Weight	Approx. 5.8 kg		
Operation temperature/humidity range	13 to 33°C, relative humidity 80 % or less (at 33°C) with no condensation		
Storage temperature/humidity range	0 to 40°C, relative humidity 80 % or less (at 35°C) with no condensation		

*1 USB memory devices with no security features are supported.

*2 USB human interface device class US layout keyboards are supported. (Operation is not guaranteed for all of the above supported USB memories and keyboards.)




SAFETY PRECAUTIONS

For correct use and for your safety, be sure to read the instruction manual before using the instrument.


- Always connect the instrument to the specified power supply voltage. Improper connection may cause a fire or electric shock.

- The specifications and appearance shown herein are subject to change without notice.
- If you have any questions about specifications, please contact your Konica Minolta representative.
- Konica Minolta, the Konica Minolta logo and symbol mark, and "Giving Shape to Ideas" are registered trademarks or trademarks of KONICA MINOLTA, INC.

ISO Certifications of KONICA MINOLTA, Inc., Sakai Site



JQA-QMA15888
Design, development, manufacture/
manufacturing management, calibration, and
service of measuring instruments



JQA-E-80027
Design, development,
manufacture, service and sales
of measuring instruments

KONICA MINOLTA, INC.	Osaka, Japan		
Konica Minolta Sensing Americas, Inc.	European HQ / BENELUX	PHONE: (888)473-2656 (in USA), +1(201)236-4300 (outside USA)	FAX: +1(201)785-2480 E-Mail: service.sus@konicaminolta.com
Konica Minolta Sensing Europe B.V.	German Office	PHONE: +31(0)30 248-1193	E-Mail: info.benelux@seu.konicaminolta.eu
	French Office	PHONE: +49(0)89 4357 156 0	E-Mail: info.germany@seu.konicaminolta.eu
	UK Office	PHONE: +33(0)1 80 11 10 70	E-Mail: info.france@seu.konicaminolta.eu
	Italian Office	PHONE: +44(0)1925 467300	E-Mail: info.uk@seu.konicaminolta.eu
	Swiss Office	PHONE: +39 02849488.00	E-Mail: info.italy@seu.konicaminolta.eu
	Nordic Office	PHONE: +41(0)43 322-9800	E-Mail: info.switzerland@seu.konicaminolta.eu
Konica Minolta (CHINA) Investment Ltd.	Polish Office	PHONE: +46(0)31 7099464	E-Mail: info.nordic@seu.konicaminolta.eu
	SE Sales Division	PHONE: +48(0)71 73452-11	E-Mail: info.poland@seu.konicaminolta.eu
	Beijing Office	PHONE: +86(0)21-6057-1089	E-Mail: hcn_sensing@gcp.konicaminolta.com
	Guangzhou Office	PHONE: +86(0)10-8522 1551	E-Mail: hcn_sensing@gcp.konicaminolta.com
	Chongqing Office	PHONE: +86(0)20-3826 4220	E-Mail: hcn_sensing@gcp.konicaminolta.com
	Qingdao Office	PHONE: +86(0)23-6773 4988	E-Mail: hcn_sensing@gcp.konicaminolta.com
Konica Minolta Sensing Singapore Pte. Ltd.	Wuhan Office	PHONE: +86(0)532-8079 1871	E-Mail: hcn_sensing@gcp.konicaminolta.com
	Shenzhen Office	PHONE: +86(0)27-6885 0586	E-Mail: hcn_sensing@gcp.konicaminolta.com
	Xi'an Office	PHONE: +86(0)755-2868 7535	E-Mail: hcn_sensing@gcp.konicaminolta.com
	Xiamen Office	PHONE: +86(0)592-7107 399	E-Mail: hcn_sensing@gcp.konicaminolta.com
	Singapore	PHONE: +65 6563-5533	E-Mail: se-service.sg@konicaminolta.com
	Korean HQ	PHONE: +82(0)2-523-9726	E-Mail: se.korea@konicaminolta.com
Konica Minolta Sensing Korea Co., Ltd.	Cheonan Office	PHONE: +82(0)41-556-9726	E-Mail: se.korea@konicaminolta.com

Addresses and telephone/fax numbers and e-mail address are subject to change without notice.
For the latest contact information, please refer to KONICA MINOLTA Worldwide Offices web page:

<https://konicaminolta.com/instruments/network>