


### 3-in-1 next-generation measurement tool

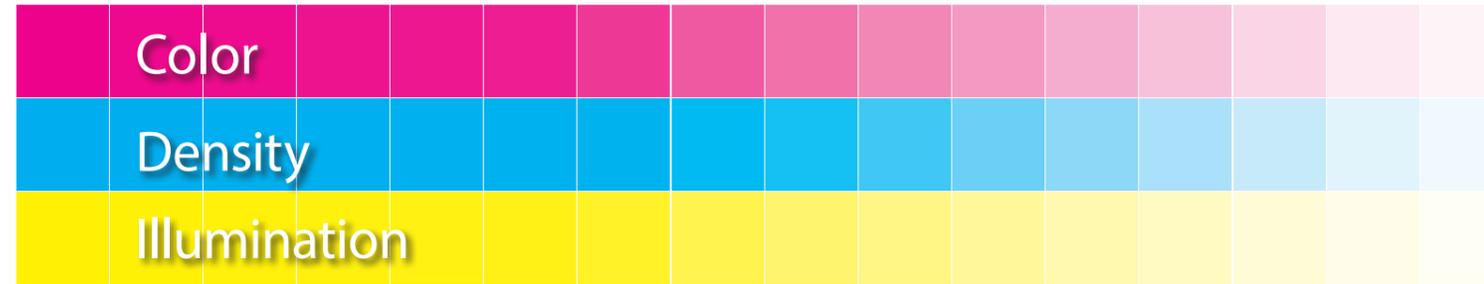

Function	FD-7	FD-5
<b>Density measurement functions</b>		
Density, density difference	●	●
Dot area	●	●
Dot gain	●	●
Trapping	●	●
PS plate dot area	●	●
PS plate dot gain	●	●
Spot color density	●	●
Gray balance	●	●
Midtone spread	●	●
ISO 12647 check	●	●
Target match	●	●
<b>Colorimetric measurement functions</b>		
L*a*b*	●	●
L*C*h	●	●
Hunter Lab	●	●
Yxy	●	●
XYZ	●	●
ΔE* <sub>ab</sub> (CIE1976)	●	●
ΔE* <sub>94</sub> (CIE1994)	●	●
ΔE <sub>00</sub> (CIE2000)	●	●
ΔE (Hunter)	●	●
CMC (l:c)	●	●
<b>Illuminance measurement functions</b>		
Illuminance*1	●	
Correlated color temperature	●	
<b>Paper index</b>		
WI/Tint (ASTME313-96)	●	●
ISO Brightness (ISO2470-1)	●	●
D <sub>65</sub> Brightness (ISO2470-2)	●	●
Fluorescence index	●	●
<b>Spectral reflectance</b>		
Spectral data output	●	
<b>Memory</b>		
Target density	30	30
Target color	30	30
Color sets of 15 colors each*2	50	50
<b>Other functions</b>		
Manual scan*3	●	
Automatic function (density, dot area, color)	●	●
PASS/FAIL judgment	●	●
<b>Software</b>		
FD-S1w	●	●
SpectraMagic NX	●	●
ClrChrt (Included with ColorScout series)	●	●

Main specifications	
Illumination/viewing system	45°a: 0°(annular illumination)** Conforms to CIE No. 15, ISO 7724/1, DIN5033 Teil 7, ASTM E 1164, and JIS Z 8722 Condition a for reflectance measurements.
Spectral separation device	Concave grating
Wavelength range	Spectral reflectance: 380 to 730 nm; Spectral irradiance (FD-7 only): 360 to 730 nm
Wavelength pitch	10 nm
Half bandwidth	Approx. 10 nm
Measurement area	Ø3.5 mm
Light source	LED
Measurement range	Density: 0.0D to 2.5D; Reflectance: 0 to 150%
Repeatability	Density: σ0.01D Without polarization filter: 0.0D ~ 2.5D, Yellow 0.0D ~ 2.0D With polarization filter: 0.0D ~ 2.5D, Yellow 0.0D ~ 1.8D (When measurements taken 30 times at 10-second intervals after white calibration has been performed) Colorimetric: Within σΔE <sub>00</sub> 0.05 (Without polarization filter) (When white calibration plate is measured 30 times at 10-second intervals after white calibration has been performed)
Inter-instrument agreement	Within ΔE <sub>00</sub> 0.3 (Average of 12 BCRA Series II color tiles compared to values measured with a master body under Konica Minolta standard conditions; without polarization filter)
Measurement time	Approx. 1.4 s (single-point reflectance measurement without polarization filter)
Battery performance	Approx. 2,000 (when new without polarization filter)
Measurement conditions*5	M0 (A), M1 (D50), M2 (A + UV-cut filter), and M3 (M2 + polarization filter); User-defined illuminant
Illuminant	A, C, D50, D65, ID50, ID65, F2, F6, F7, F8, F9, F10, F11, F12, User-defined illuminant
Observer	2° or 10° Standard Observer
Density	ISO Status T, ISO Status E, ISO Status A, ISO Status I; DIN16536
Display language	English, French, German, Spanish, Japanese, Chinese (Simplified)
Interface	USB 2.0
Output data*3	Displayed values; Spectral reflectance data (FD-7 only); Spectral irradiance data (FD-7 only)
Power	Rechargeable internal lithium-ion battery; AC adapter; USB bus power
Size (W × D × H)	70 × 165 × 83 mm (Body only); 90 × 172 × 84 mm (With target mask attached)
Weight	Approx. 350 g (Body only); Approx. 430 g (With target mask attached)
Operation temperature/humidity range	10 to 35°C, 30 to 85% relative humidity with no condensation
Storage temperature/humidity range	0 to 45°C, 0 to 85% relative humidity with no condensation

\*1 Simple illuminance measurement function. Does not conform to JIS standards.  
 \*2 Used for ISO 12647 Check / Target match; Must be set using included FD-S1w software.  
 \*3 Available when using PC software.  
 \*4 Illumination for wavelengths under 400nm is unidirectional.  
 \*5 M0, M1, M2: Illumination conditions defined in ISO 13655 4.2.2 Illumination requirements and measurement conditions.  
 •Displays shown are for illustration purpose only.  
 •The specifications and appearance shown herein are subject to change without notice.  
 •KONICA MINOLTA, the Konica Minolta logo and symbol mark, "Giving Shape to Ideas" and SpectraMagic are registered trademarks or trademarks of KONICA MINOLTA, INC.  
 •Other company names and product names used herein are trademarks or registered trademarks of their respective companies.



**SAFETY PRECAUTIONS**  
 For correct use and for your safety, be sure to read the instruction manual before using the instrument.  
 ● Always connect the instrument to the specified power supply voltage. Improper connection may cause a fire or electric shock.

ISO Certifications of KONICA MINOLTA, Inc., Sakai Site



JQA-QMA15888 Design, development, manufacture/  
 manufacturing management, calibration, and service of measuring instruments  
 JQA-E-80027 Design, development, manufacturing management, calibration, service and sales of measuring instruments

KONICA MINOLTA, INC.  
 Konica Minolta Sensing Americas, Inc.  
 Konica Minolta Sensing Europe B.V.

Osaka, Japan  
 New Jersey, U.S.A.  
 European Headquarter /BENELUX  
 German Office  
 French Office  
 UK Office  
 Italian Office  
 Swiss Office  
 Nordic Office  
 Polish Office  
 Turkish Office  
 SE Sales Division  
 Beijing Office  
 Guangzhou Office  
 Chongqing Office  
 Qingdao Office  
 Wuhan Office

Phone : 888-473-2656 (in USA), 201-236-4300 (outside USA)  
 Nieuwegein, Netherlands  
 München, Germany  
 Roissy CDG, France  
 Warrington, United Kingdom  
 Cinisello Balsamo, Italy  
 Dietikon, Switzerland  
 Västra Frölunda, Sweden  
 Wrocław, Poland  
 Istanbul, Turkey  
 Shanghai, China  
 Beijing, China  
 Guangdong, China  
 Chongqing, China  
 Shandong, China  
 Hubei, China  
 Singapore  
 Goyang-si, Korea

Fax : 201-785-2482  
 +31 (0) 30 248-1193  
 +49 (0) 89 4357 156 0  
 +33 (0) 1 80 11 10 70  
 +44 (0) 1925 467300  
 +39 02849488.00  
 +41 (0) 43 322-9800  
 +46 (0) 31 7099464  
 +48 (0) 71 73452-11  
 +90 (0) 216-528 56 56  
 +86 (0) 21-5489 0202  
 +86 (0) 10-8522 1551  
 +86 (0) 20-3826 4220  
 +86 (0) 23-6773 4988  
 +86 (0) 532-8079 1871  
 +86 (0) 27-8544 9942  
 +65 6563-5533  
 +82 (0) 2-523-9726

Konica Minolta (CHINA) Investment Ltd.  
 Konica Minolta Sensing Singapore Pte Ltd.  
 Konica Minolta Sensing Korea Co., Ltd.  
 Addresses and telephone/fax numbers are subject to change without notice. For the latest contact information, please refer to the KONICA MINOLTA Worldwide Offices web page :  
 ©2010 KONICA MINOLTA, INC.

<https://konicaminolta.com/instruments/network>  
 9242-A3E2-41 CABPK



Streamlines color adjustment in printing, even on substrates with fluorescent whitening agents

# A high-accuracy, compact, lightweight, handheld, next-generation spectrophotometer that measures color, density, and illumination\* for applications from R&D to quality control. \*FD-7 only

## Color

### The world's first measuring instrument that corresponds to Measurement Condition M1 of ISO 13655

- Konica Minolta's original VFS (Virtual Fluorescence Standard) technology enables L\*a\*b\* measurements corresponding to ISO 13655 Measurement Condition M1.
- The FD-7 and FD-5 can take measurements corresponding to all four of the ISO 13655 Measurement Conditions. Measurements corresponding to M1 are enabled by Konica Minolta's original VFS (Virtual Fluorescence Standard) technology, and measurements corresponding to M0 (CIE Illuminant A) and M2 (illumination with UV-cut filter) can also be taken. In addition, by attaching the included polarization filter, measurements corresponding to M3 (M2+ polarization filter) can be taken.

### Scan measurements can be performed. (FD-7 only)

- Manual scan measurements can be performed when the instrument is connected to a PC.

### Spectral output (FD-7 only)

- When the FD-7 is connected to a computer, the spectral reflectance data (380 to 730 nm) of samples under various illuminants and the spectral irradiance data (360 to 730 nm) of the environmental lighting can be measured and output to a computer. This makes the FD-7 ideal for research and development applications.



By measuring the environmental light source with an FD-7 master body and then transferring the user illuminant data to multiple FD-5 or FD-7 working bodies, color control using the same illumination light source at multiple locations can be achieved. In addition, the automatic wavelength compensation function minimizes inter-instrument errors when using multiple instruments.

FD-5 (Working body)



FD-5 (Working body)



### Data Management Software FD-S1w (included as standard accessory)

**Features:**

- Transfer of measurement data to Excel® sheet.
- Reading/registration of user illuminant data to/and storage as PC file
- Color set management functions (for instrument and Target Match functions)\*\*2\*3

**System Requirements**

**OS** Windows® 7 Professional 32-bit, 64-bit  
Windows® 8.1 Pro 32-bit, 64-bit  
Windows® 10 Pro 32-bit, 64-bit

**Excel** Excel® 2010 32-bit (Windows® 7)  
Excel® 2013 (Windows® 8.1, Windows® 10)  
Excel® 2016 (Windows® 10)  
\* Excel® 2010 must be 32-bit version.  
The hardware or the computer system to be used must meet or exceed the recommended system requirements for the compatible OS and Excel version being used.

**Compatible Instruments** Spectrophotometer FD-7, FD-5

**Display language** English, Japanese, Chinese (Simplified)  
(Select one during installation.)

**FD-S1w.exe**



## Illumination

### Illumination environment light can be measured. (FD-7 only)

- The illuminance<sup>1</sup> and color temperature in a color viewing cabinet or the actual ambient light under which printed materials will be evaluated can be measured.

### Measured environmental light can be set as illumination light source (user-defined illuminant)

- In the past, when measuring printed materials containing fluorescent whitening agents (FWA), large differences between measured values and visual evaluation sometimes occurred. But with the FD-7, colorimetric values can be calculated under the measured environmental light source, providing results which more closely correspond to on-site visual evaluation. This ensures customers receive the colors they want and eliminates time and labor lost resolving customer complaints due to the effects of FWA or metamerism.

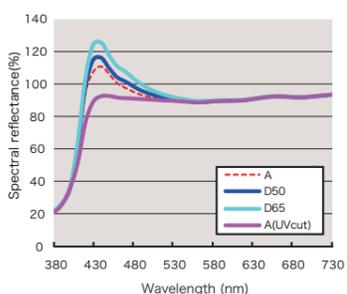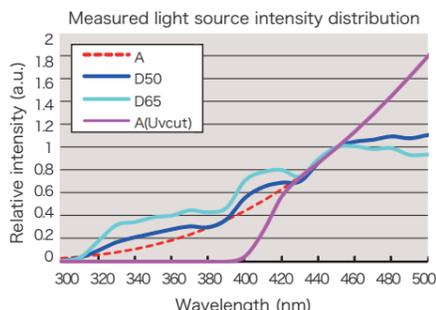

## Density

### Printing quality control functions including trapping, dot gain, etc.

- A new industry-standard tool for commercial printing and packaging printing to improve productivity and quality at low cost.

- CMYK density • Dot area • Dot gain • Trapping • Simple density difference
- PS plate dot area • PS plate dot gain • Spot color density

Improvements in quality control functions to meet more advanced needs at printing locations.



### Target Match function\*\*2\*3


- Displays the color difference from the target color and the process color or spot color density adjustment needed to bring the measured color closer to the target color. By using the Target Match function, ink color adjustment can be performed without a computer or special software.
- Ideal for spot colors or process colors.
- Displays color difference and density.
- Displays estimated density adjustment needed to bring the measured color closer to the target color and the predicted color difference after adjustment.

Measure color difference. Result: Adjusting the density of spot color with 400 nm peak absorbance from 0.86 to 1.16 is predicted to result in a color difference of 0.48.

TARGETMATCH	M1 2° D50	
<input checked="" type="checkbox"/> Paper	ΔD(400)	+0.30 D
<input checked="" type="checkbox"/> Target	ΔE*94	
<input checked="" type="checkbox"/> Sample	2.54 @ 0.86 D	
	>> 0.48 @ 1.16 D	
Measure sample		

### Functions corresponding to various printing standards

- Pass/fail judgment against ISO, JapanColor, GRACoL®/SWOP®, PSO, or user-defined custom targets can be performed. The FD-7 and FD-5 are ideal for on-site printing quality control.
- ISO 12647 check\*\*2\*3  
Color difference, TVI, and mid-tone spread can be evaluated.
- Gray balance  
Gray balance can be evaluated using the G7® evaluation method.

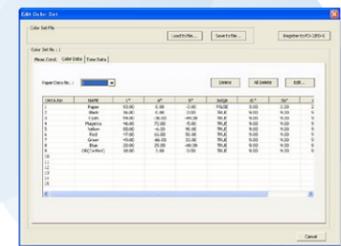

ISO CHECK	M1 2° D50	
<input checked="" type="checkbox"/> Yellow40%	ΔL*	-0.32
<input checked="" type="checkbox"/> Red	Δa*	0.08
<input checked="" type="checkbox"/> Green	Δb*	-0.22
<input type="checkbox"/> Blue	ΔE*ab	0.40
	16/21	CS01 : PT1-AM-BB
Red : Pass		

\*\*2 Target colors (color sets) must be set using the included FD Data Management Software FD-S1w.  
\*\*3 Backing conversion function converts the target values to enable evaluation even when backing conditions for samples do not match those of the targets.

\*1 Simple illuminance measurement function. Does not conform to JIS standards.

## Industry's first automatic wavelength compensation function

- Wavelength compensation is performed during white calibration<sup>\*3</sup> without requiring additional work.
- Until now, wavelength compensation could only be carried out as one part of manufacturer servicing. This task is now performed whenever white calibration<sup>\*3</sup> is done, helping to maintain the high reliability of measurement values until the next periodic servicing.

\*3 Except when polarization filter is attached.


## World's lightest<sup>\*4</sup>

- The main body weighs only about 350g, and even with the target mask attached it's only about 430g, lighter than any previous spectrodensitometer.
- This reduces the load on the user's arm during work, improving efficiency when taking measurements over a long time.


\*4 Display-equipped spectrodensitometer. As of December 1, 2012

## Worry-free after-sales service

- Worldwide service centers provide rapid support when needed.
- A comprehensive service network is in place to ensure that your instrument is always in top shape.

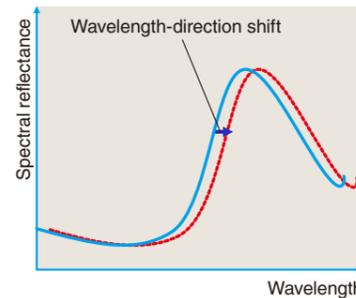


## System Diagram

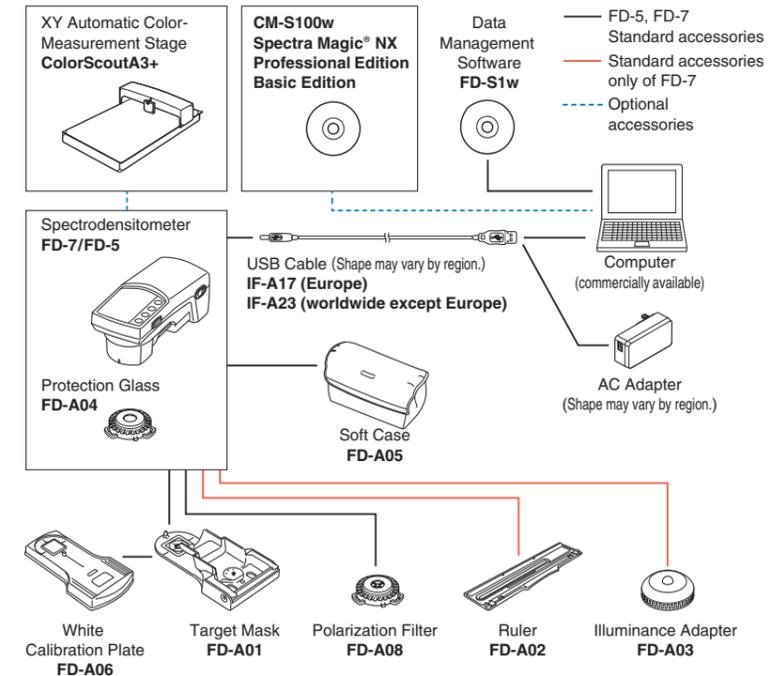

## Dimensions (Units: mm)

With removable target mask attached

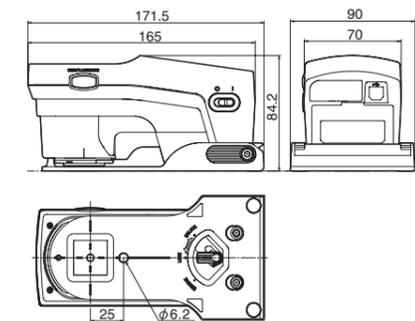

## Optional accessories

\*5 Measurements with polarization filter attached cannot be performed.

## XY Automatic Color-Measurement Stage ColorScout series<sup>\*5</sup>

The ColorScout series enables accurate, high-efficiency measurements of color charts with the Spectrodensitometer FD-7 and FD-5. It enables automatic positioning and measurement of the instrument, providing higher repeatability and reducing labor compared to manual measurements.


**XY automatic color-measurement stage**  
Backing sheet available as either white surface or black surface.



## Capable of both spot and scan measurements!

- Supports A3+ and A4+ sizes. Measurements can be efficiently done without cutting, folding and switching in and out important color charts
- Definition files can be easily created for charts using the ClrChrt application that comes standard with the product.
- Data can be saved in ANSI8.7 or CGATS.5 format and exported to profile editing software. Colors can be reproduced closer to what is perceived with the human eye, by using M1 light sources or user-defined light sources.
- The ES series uses electrostatic attraction to immobilize charts during measurement.

## ClrChrt software (Included)

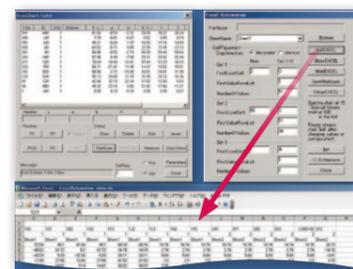

Measurement data

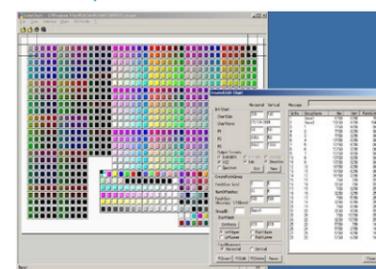


Chart design screen

Specification	ColorScout A3+	ColorScout A3+ ES	ColorScout A4+ ES
Electrostatic attraction	-	✓	✓
Measureable sizes	320 x 460 mm	320 x 460 mm	320 x 230 mm
Sample thickness	Max 1.5 mm	Max 1.0 mm	Max 1.0 mm


ColorChart minimum computing requirements	
OS; CPU	Windows®7(32-bit, 64-bit); 300MHz or faster
Hard disk; Memory	30MB or more available disk space; 64MB or more

## Color Data Software SpectraMagic NX<sup>\*5</sup>


Ideal for color-difference control of spot colors relative to target colors.

## Achieves overall ease of use with free selection of evaluation equations and report formatting.


With the new E\*<sub>94</sub> and E<sub>00</sub> color difference equations as well as a user index that allows users to freely set their own evaluation equations, SpectraMagic NX can meet a wide variety of user needs. Measurement data can be displayed in list form or in objects such as spectral graphs, color-difference graphs, etc. that the user can freely lay out, and those objects can be copied and pasted as is into other software such as Excel® for easy data control. In addition, printing screens can also be designed using the same objects to create user-defined formats for easy-to-read reports.




List display



Color-difference graph object

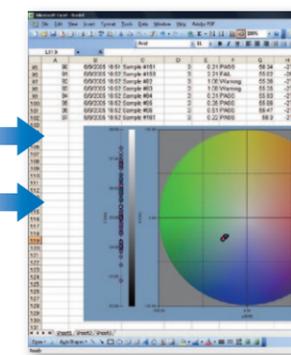

Pasted into Excel®

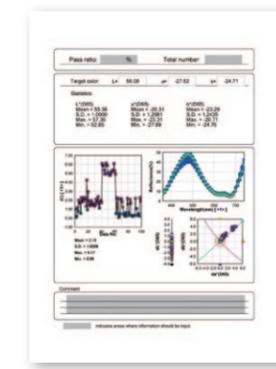

Printing screen

Minimum Computing Requirements	
OS	Windows® 7 Professional 32-bit, 64-bit; Windows® 8.1 Pro 32-bit, 64-bit; Windows® 10 Pro 32-bit, 64-bit (English, Japanese, German, French, Spanish, Italian, Traditional Chinese, Simplified Chinese, Portuguese, and Hanguk versions) • The hardware of the computer system to be used must meet or exceed the greater of the recommended system requirements for the compatible OS being used or the following specifications.
CPU	Pentium® III 600 MHz or higher (recommended)
Memory	128 MB (256 MB recommended)
Hard disk	450 MB of available disk space (At least 400 MB of available space is required in the system drive.)